Because we care.

MIDMARK®

Installation / Operation

Blood Drawing Chair
Model 165-005 w/ Swing Arms
Model 165-006 w/ Swing Arms and Drawer

KIT COMPONENTS

Part Number	Description	Qty
165-005	Chair w/ two lockable, swing arms	1
165-006	Chair w/ lockable, swing arms and drawer	1
• 003-1084-00	Installation / Operation Instructions	1

REQUIRED TOOLS

Tools required to change drawer assembly between Right-hand and Left-hand chair side:

Phillips Screwdriver
1/2" Socket and Ratchet

INTRODUCTION

Chair provided with rotational arms, lockable in ten positions, for purpose of drawing blood.
Chair can be ordered with an optional right or left-hand drawer / swing arm assembly.
Maximum drawer weight capacity 20 lbs. (9.1 Kgs.)

INSTALLATION

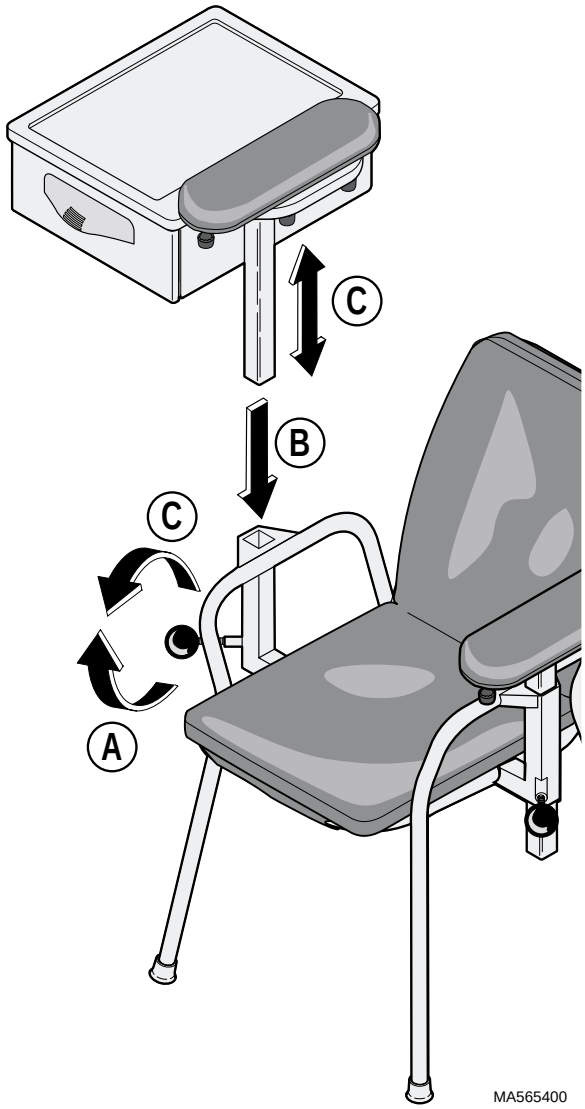

NOTE

Model 165-005 is completely assembled.
Model 165-006 Chair must have the drawer assembly installed.

- **A.** Loosen knob.
- **B.** Insert drawer post into receptacle on chair side.
- **C.** Adjust height and tighten knob.

© Midmark Corporation - 2000

REORIENTING DRAWER

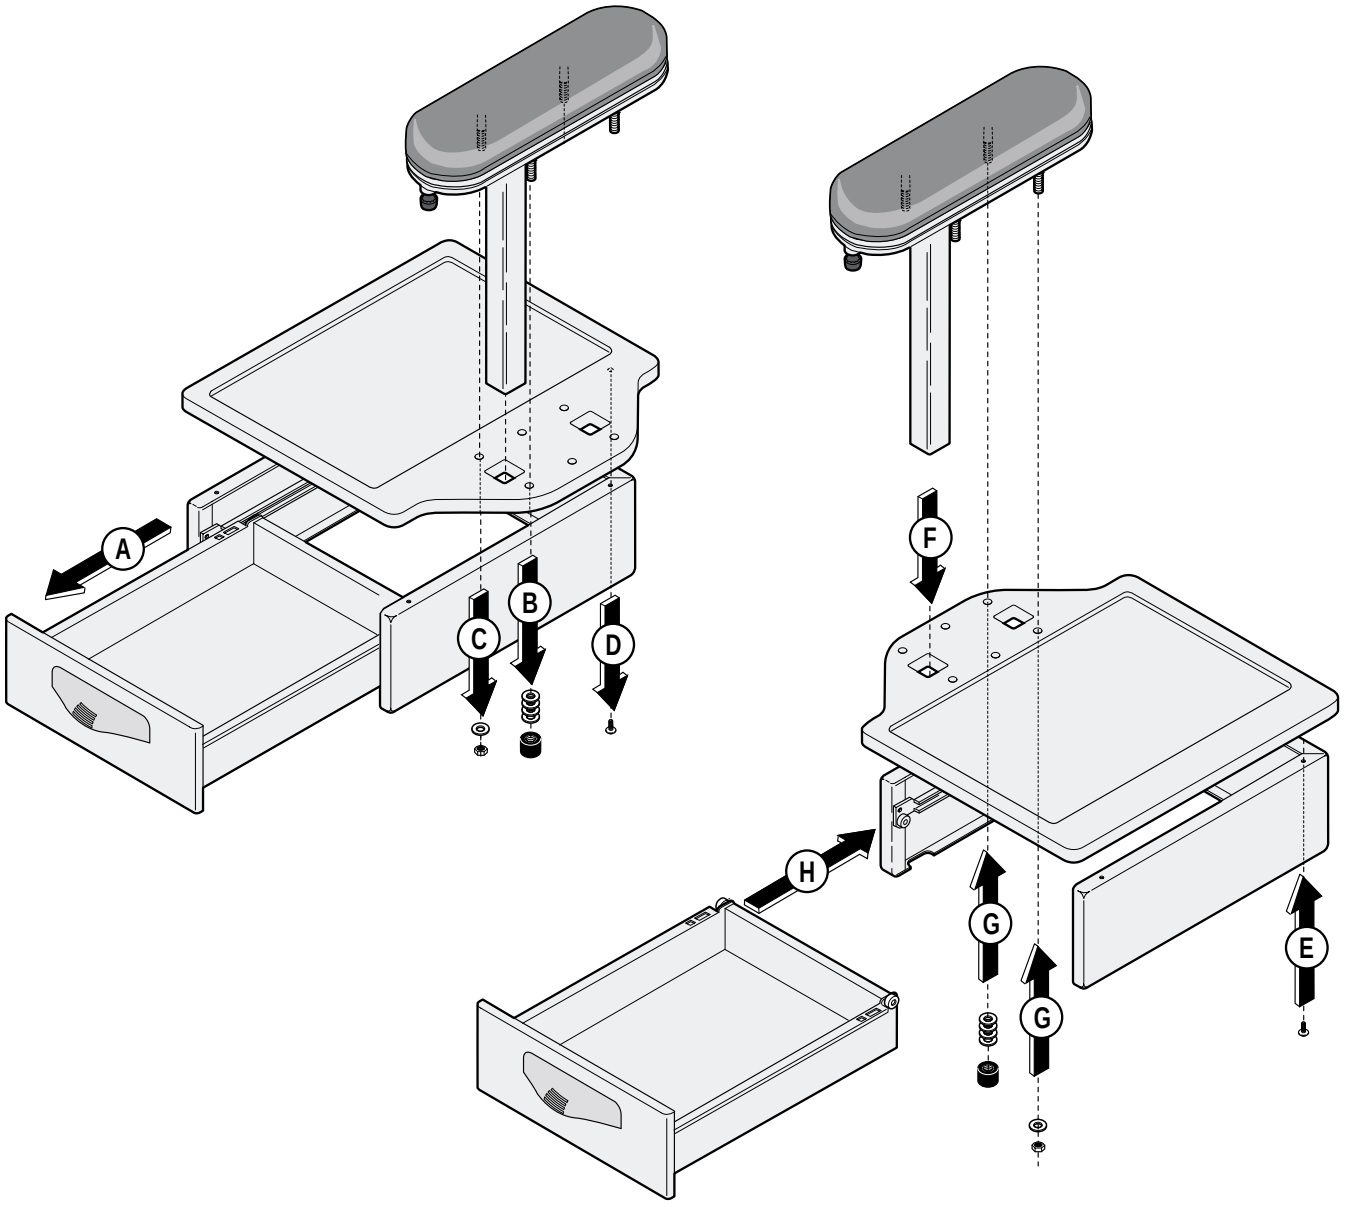

MA565500

NOTE

To change position of drawer assembly between right-hand and left-hand chair side, complete the following steps:

- **A.** Remove drawer.
- **B.** Remove two bumpers and eight washers.
- **C.** Remove two nuts and two washers, then separate Arm Assembly from top.
- **D.** Separate drawer housing from drawer top (four screws).
- **E.** Rotate top 180° and secure to drawer housing (four screws)
- **F.** Position arm assembly with indexing plunger located toward drawer housing front. Insert arm post in hole near front of drawer cover.
- **G.** Secure arm assembly with two bumpers, eight washers, two nuts and two washers.
- **H.** Install drawer.

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

© Midmark Corporation - 2000